



**Figure 1**

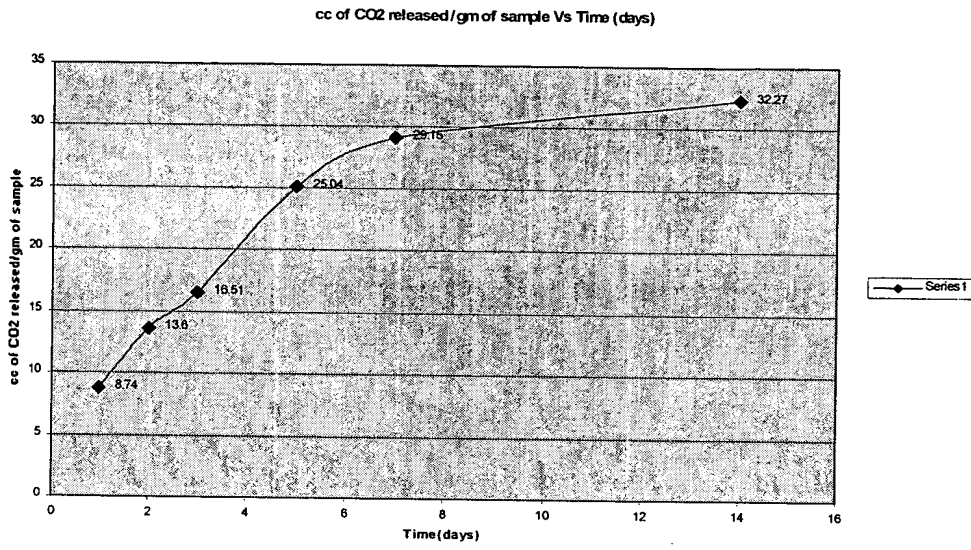

1003397 14501  
105721 265001


**Figure 2**

Leakproof vials (control samples)  
% of oxygen inside vials Vs Time (Days)

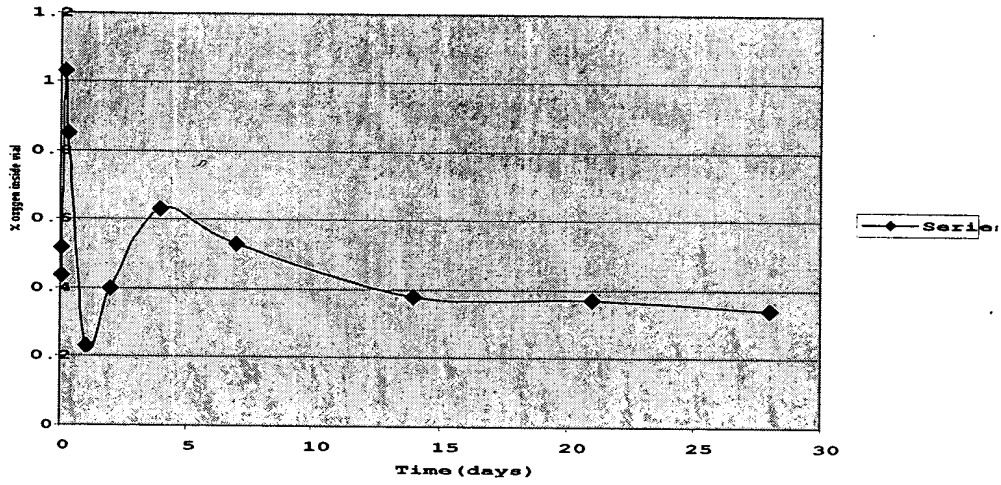

10033973 121901

# CO<sub>2</sub> release by the film X1147 (Sodium bicarbonate with malic acid)

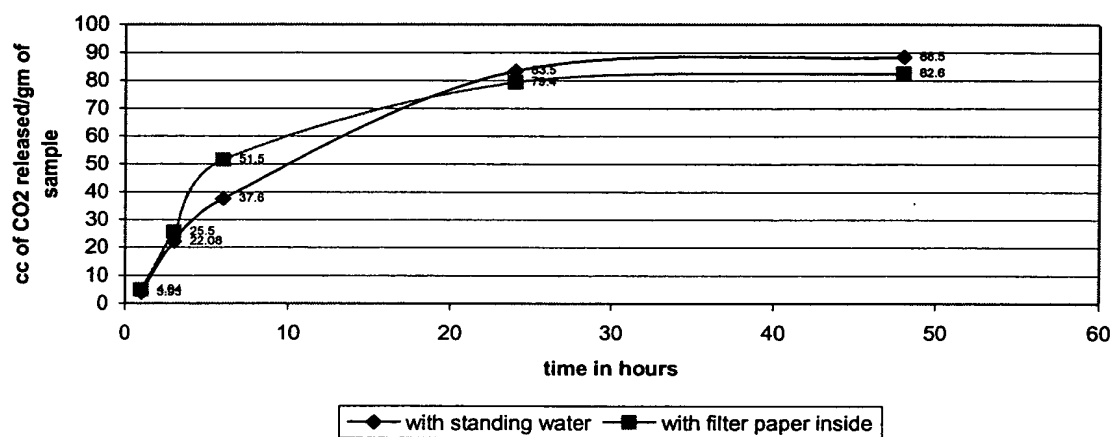

**FIGURE 3**